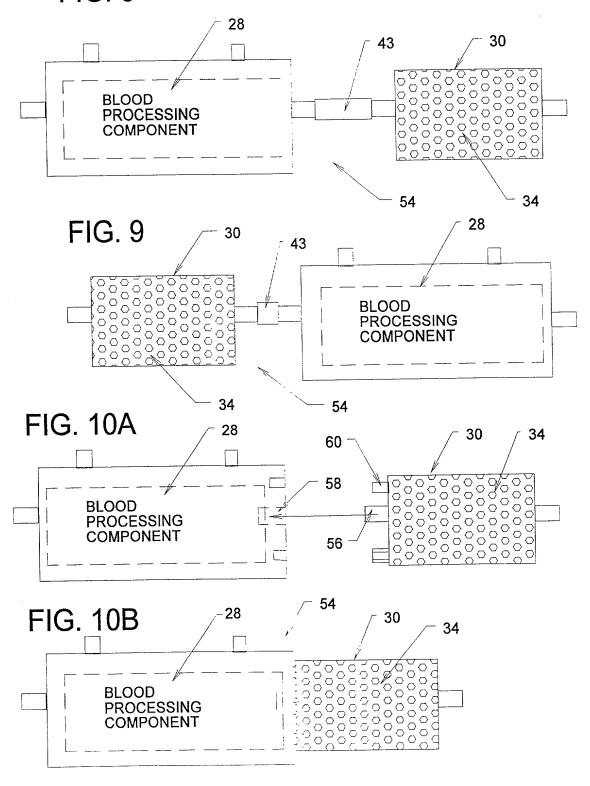


FIG. 8







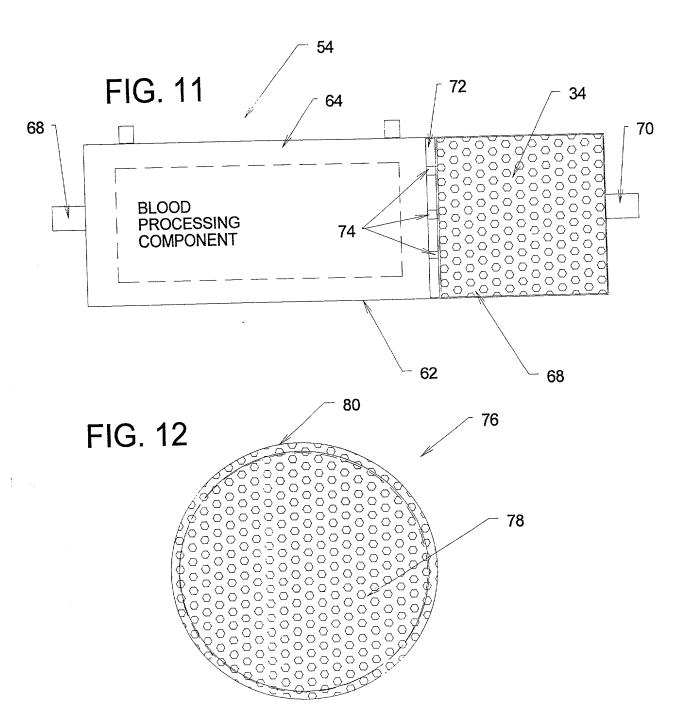


FIG. 14

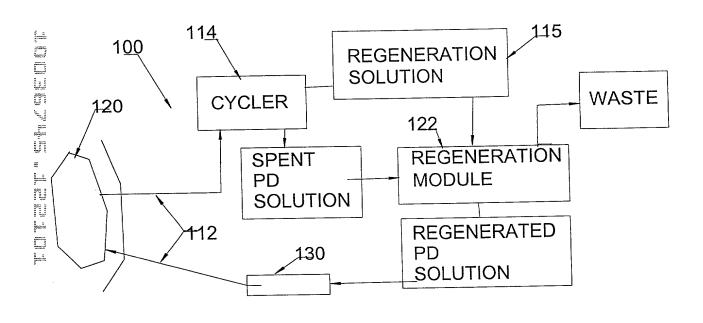


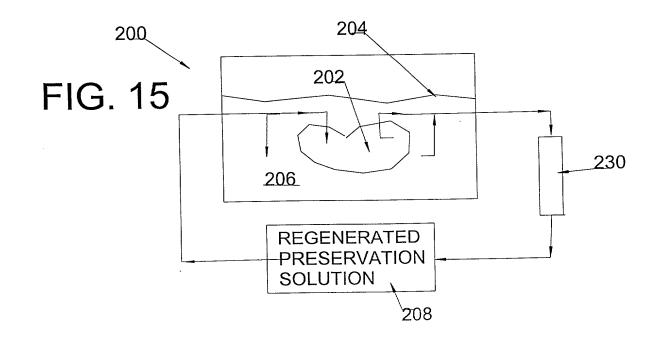

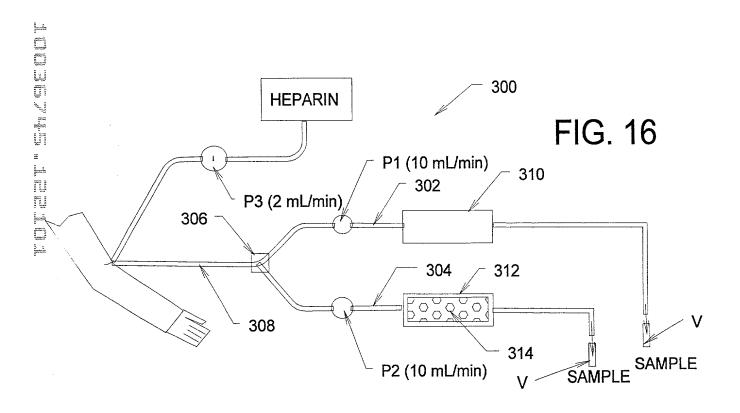

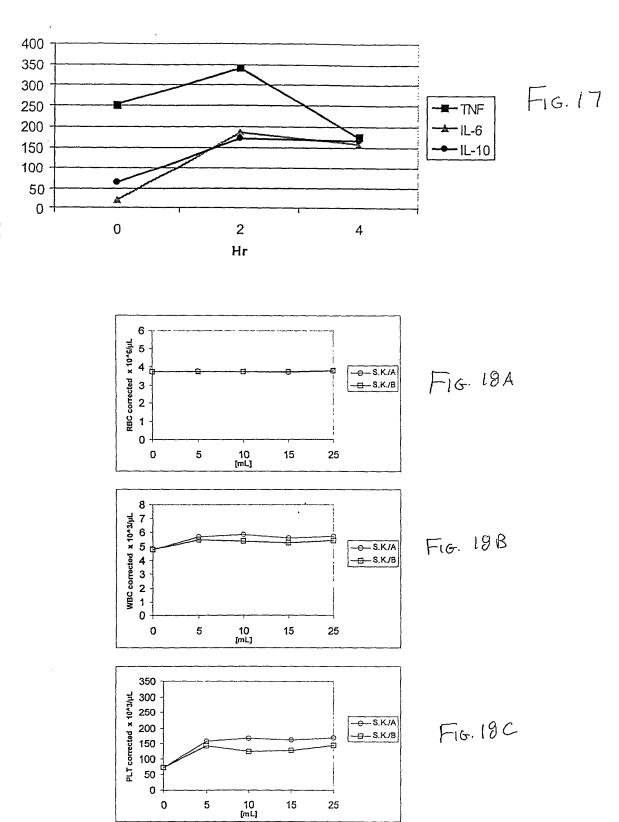

[mL]

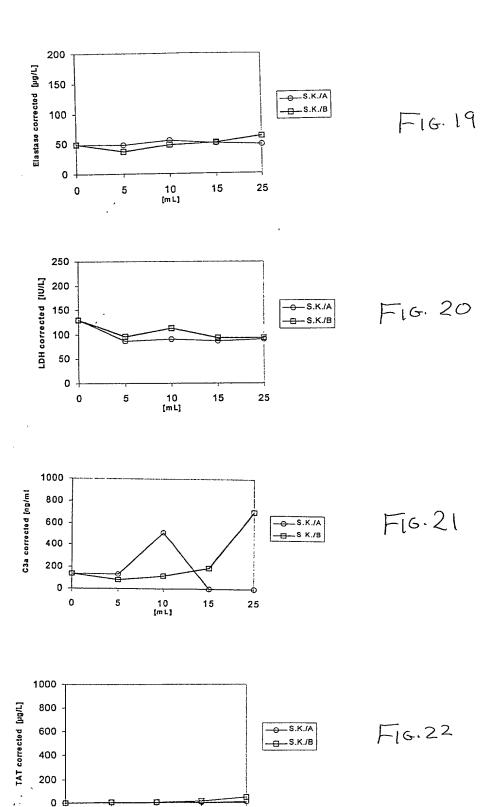

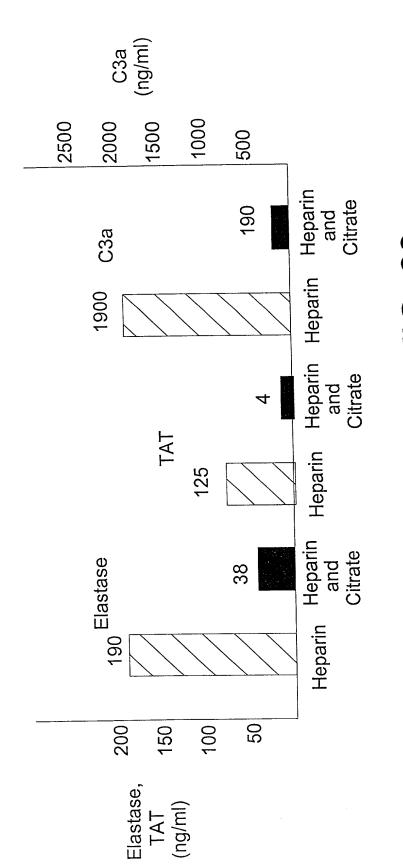


FIG. 23